


RMA device "S" output

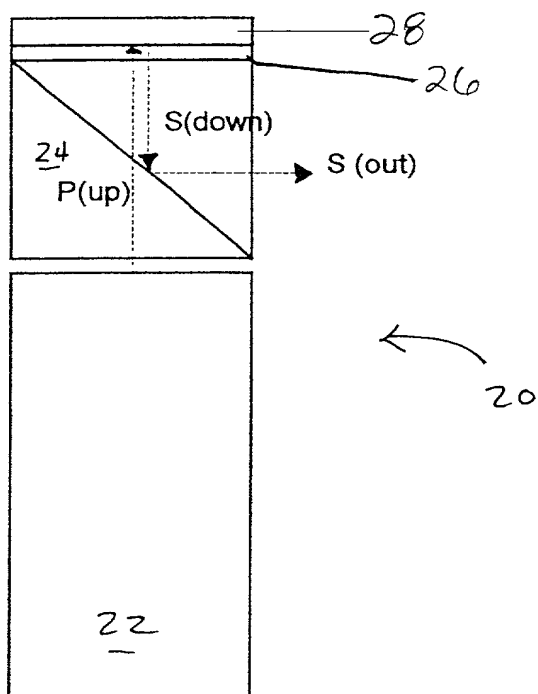

RMA device "P" output

FIG. 3

30

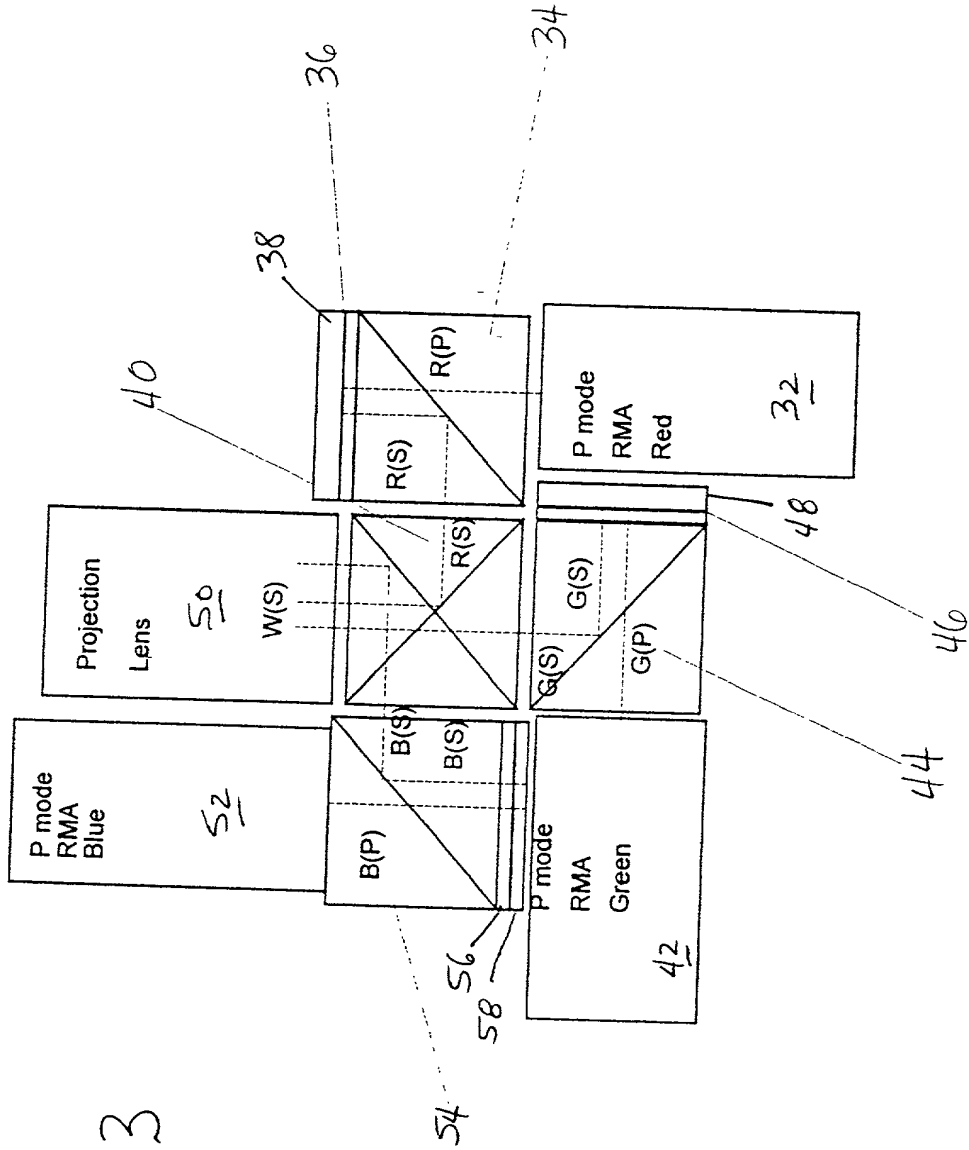


FIG. 4

100

